

Stewart, Jill, Stewart, Paul, Walker, Tom, Viramontes-Hörner, Daniela, Lucas, Bethany, White, Kelly, Taal, Maarten W., Selby, Nicholas M. and Morris, Mel (2021) An iterative run-to-run learning model to derive continuous brachial pressure estimates from arterial and venous lines during dialysis treatment. *Biomedical Signal Processing and Control*, 65 . p. 102346.

Downloaded from: <http://insight.cumbria.ac.uk/id/eprint/7088/>

Usage of any items from the University of Cumbria's institutional repository 'Insight' must conform to the following fair usage guidelines.

Any item and its associated metadata held in the University of Cumbria's institutional repository Insight (unless stated otherwise on the metadata record) may be copied, displayed or performed, and stored in line with the JISC fair dealing guidelines (available [here](#)) for educational and not-for-profit activities

provided that

- the authors, title and full bibliographic details of the item are cited clearly when any part of the work is referred to verbally or in the written form
 - a hyperlink/URL to the original Insight record of that item is included in any citations of the work
- the content is not changed in any way
- all files required for usage of the item are kept together with the main item file.

You may not

- sell any part of an item
- refer to any part of an item without citation
- amend any item or contextualise it in a way that will impugn the creator's reputation
- remove or alter the copyright statement on an item.

The full policy can be found [here](#).

Alternatively contact the University of Cumbria Repository Editor by emailing insight@cumbria.ac.uk.

An Iterative Run-to-Run Learning Model to Derive Continuous Brachial Pressure Estimates from Arterial and Venous Lines During Dialysis Treatment

Jill Stewart, Paul Stewart, *Senior Member, IEEE*, Tom Walker, Daniela Viramontes Horner, Bethany Lucas, Kelly White, Maarten W Taal and Nicholas M Selby .

Abstract

Objective: Non-invasive continuous blood pressure monitoring is not yet part of routine practice in renal dialysis units but could be a valuable tool in the detection and prevention of significant variations in patient blood pressure during treatment. Feasibility studies have delivered an initial validation of a method which utilises pressure sensors in the extra-corporeal dialysis circuit, without any direct contact with the person receiving treatment. Our main objective is to further develop this novel methodology from its current early development status to a continuous-time brachial artery pressure estimator.

Method: During an *in vivo* patient feasibility study with concurrent measurement validation by *Finapres Nova* experimental physiological measurement device, real-time continuous dialysis line pressures, and intermittent occluding arm cuff pressure data were collected over the entire period of (typically 4-hour) dialysis treatments. There was found to be an underlying quasi-linear relationship between arterial line and brachial pressure measurements which supported the development of a mathematical function to describe the relationship between arterial dialysis line pressure and brachial artery BP. However, unmodelled non-linearities, dynamics and time-varying parameters present challenges to the development of an accurate BP estimation system. In this paper, we start to address the problem of physiological parameter time variance by novel application of an iterative learning run-to-run modeling methodology originally developed for process control engineering applications to a parameterised BP model.

Results: The iterative run-to-run learning methodology was applied to the real-time data measured during an observational study in 9 patients, supporting subsequent development of an adaptive real-time BP estimator. Tracking of patient BP is analysed for all the subjects in our patient study, supported only by intermittent updates from BP cuff measurements.

Conclusion: The methodology and associated technology is shown to be capable of tracking patient BP non-invasively via arterial line pressure measurement during complete 4-hour treatment sessions. A robust and tractable method is demonstrated, and future refinements to the approach are defined.

Index Terms

Blood pressure measurement, extracorporeal pressure sensors, fistula, hemodialysis, continuous blood pressure measurement model parameter optimisation, iterative learning, control engineering run-to-run control, iterative learning

I. INTRODUCTION

CONTINUOUS monitoring of blood pressure (BP) during dialysis [1] has the potential to improve patient outcomes [2]–[4] and could ultimately inform treatment regime or close a personalised therapeutic intervention loop via modulation of dialysis time and/or duration, dialysate sodium concentration and/or temperature on a per patient basis. Of particular interest is *intradialytic* hypotension (IDH), a decrease in systolic blood pressure [5], generally a relatively sudden event with associated symptoms include dizziness or fainting, muscle cramps, abdominal discomfort, nausea and vomiting, often results in truncated dialysis treatments with increased risk of cerebral ischemic incidents. IDH prediction, detection and mitigation is the primary application area of the work described in this paper.

BP monitoring is normally conducted in a clinical setting via the use of an air-filled occluding arm cuff that provides a robust, but irregular and intermittent measurement that disrupts the normal blood flow, and consequently requires a significant settling time between measurements [6]. Additionally, there are three alternative distinct methods for non-invasive monitoring of BP which have occasionally been used in research settings. Arterial applanation tonometry [7], where a transducer is positioned above a superficial artery compressing it against an underlying bone [8], has been used in cardiology and anaesthetised procedures to avoid the insertion of an arterial cannula [9], [10]. Pulse Transition Time (PTT) [11] is based on measured

Paul Stewart*, Jill Stewart, Tom Walker are with the School of Health and Social Care, University of Derby, UK *corresponding author e-mail: p.stewart1@derby.ac.uk

Maarten Taal, Nick Selby, Bethany Lucas and Daniela Viramontes Horner are with the Centre for Kidney Research and Innovation, University of Nottingham, Derby, UK and the Renal unit, Royal Derby Hospital, Derby, United Kingdom

Kelly White is with the Renal unit, Royal Derby Hospital, Derby, UK

Manuscript received ; revised .

photoplethysmography (PPG) and electrocardiogram (ECG) signals during several cardiac cycles, which may not be accurate due in part to the unaccounted physiological factors in the blood pressure regulation mechanism and reliance on accurate ECG triggering [12]. Finally, the volume clamp (or vascular unloading) method [6] utilises an inflatable finger-cuff combined with an embedded photodiode to measure the diameter of finger artery. Cuff pressure is adjusted to maintain a constant artery diameter, and the changes in cuff pressure are used to calculate a BP curve in the brachial artery. In use, patients frequently report pain or discomfort at the fingertips where cuffs are placed, and this device can be unreliable in patients with reduced blood flow to the digits, often manifest in dialysis patients [11]. All three non-invasive methods are sensitive to patient movement (especially ECG signals) [13] which would result in an unacceptable and uncomfortable restriction placed on patients during a four-hour dialysis treatment.

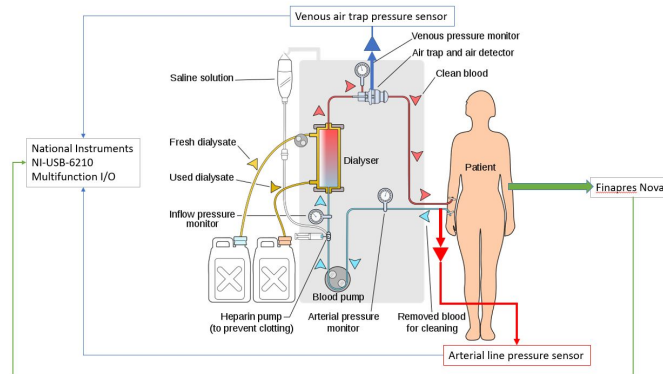


Fig. 1. Sensor and data acquisition signal flow

The iTrend (Intelligent Technologies for Renal Dialysis) programme is a long-term collaborative project performed by a multidisciplinary research team from the Universities of Derby and Nottingham and the Royal Derby Hospital Renal Unit in the UK [19], [20], developing supporting technologies, real-time analysis algorithms and heuristics to enable personalised and precision treatment in end-stage kidney disease (ESKD) [14], [15]. Blood pressure monitoring to diagnose hypertension and hypotension [16], [17] typically relies on plethorperidalytic and intermittent intradialytic BP measurements. The ability to continuously monitor BP both in terms of absolute measures and blood pressure variability could lead to new diagnostic and prognostic criteria for IDH as well as optimal and personalised treatment strategies.

A feasibility study of a novel method for continuously monitoring BP has previously been conducted (Fig.1), which introduced the placement of pressure transducers onto the venous and arterial blood lines that connect a patient to a haemodialysis machine during treatment [18], and experimentally derived relationships between pressures in these extra-corporeal blood lines and brachial BP. Pressure sensors were attached to the blood lines rather than making use of the pressure sensors present within the dialysis machines, and utilised the existing ports and connection points which are common and standardised on most dialysis blood line sets.

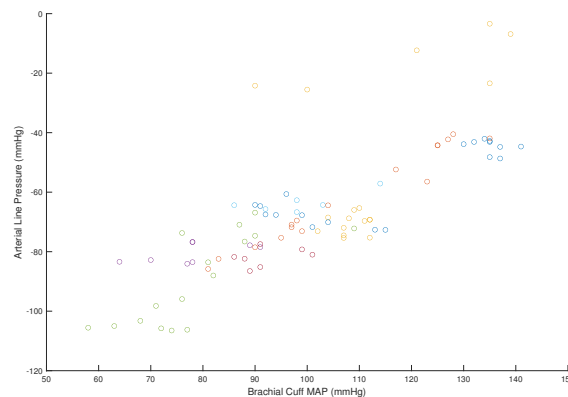


Fig. 2. Brachial cuff MAP vs Arterial line pressures in 11 patient sessions

The experimental relationship between brachial cuff MAP and corresponding measured arterial line pressure for 11 sessions in the patient study is shown in figure 2, with a linear least squares fit of

$$y = 0.8x - 1.5e + 02, \quad (1)$$

Root Mean Squares Error 10.3, R^2 0.615, p-value 6.35e-20, and is strongly associated with the physical components of the dialysis procedure (pump, pump speed, dialysis line set), with variance from the line dominated by unmodelled physiological and mechanical effects. In order to further examine this hypothesis, it is possible to negate the time varying effects in the

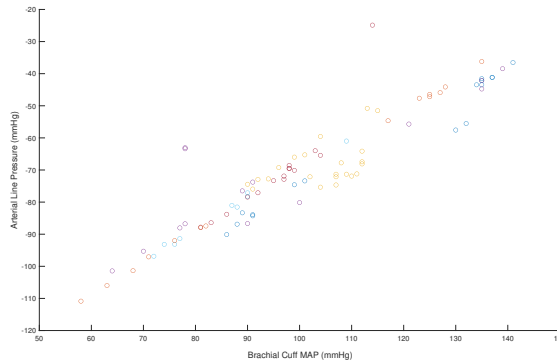


Fig. 3. Brachial cuff MAP vs Arterial line pressures in 11 patient sessions, following compensation for time varying effects during treatment

data by taking a mean value for each individual patient treatment, and recalculating the data scatter, and is shown in figure 3. A linear least squares fit of $y = 0.82x - 1.5e + 02$, Root Mean Squares Error 6.54, R^2 0.852, p-value 2.93e-38. There are a number of salient features in this plot. Firstly, the gradient of the fit has only changed by 2.5%, indicating a relatively accurate model for the machine and lines system. Secondly, the data R^2 value has risen by 38.5% to 0.852, indicating that it should be possible to design a tractable and useable time-invariant model. The feasibility study confirmed that it is potentially possible to estimate brachial BP continuously and non-invasively during the period of a dialysis session in a clinical setting with measurement of venous and arterial line pressure, and occasional measurement of brachial blood pressure by arm cuff.

A. Structure of this paper

This paper describes the development, application and performance analysis of an adaptive model parameter optimisation scheme based on iterative run-to-run learning control. The aim of this development was to compensate for the time-dependent changes of model parameters which describe the arterial line to BP relationship during 4-hour dialysis treatments. The paper is divided into the following sections:

- Section I: *Introduction*
- Section II: *Run-to-run BP Estimator* describes the application of run-to run iterative learning methodology
- Section III: *Method* describes the processing methodology for the real-time patient data sets
- Section IV: *Results* examines the effectiveness of the BP estimation scheme
- Section V: *Conclusions* assesses the overall modeling-predictor method and draws conclusions for further work

For clarity, where a patient's BP is mentioned, this should be taken to mean brachial blood pressure.

II. RUN-TO-RUN BP ESTIMATOR

The system under consideration (Fig.4) is discrete-time and non-stationary, with continuous dialysis line pressures sampled at 1kHz. This measurement constitutes the basis of calculations to estimate instantaneous, real-time BP. Patient arterial pressure is measured by occluding arm-cuff with an irregular sample rate of approximately 30 minutes, and this constitutes an accurate, repetitive measurement of BP, albeit at extremely widely spaced time-instances. The challenge addressed in this paper is to devise a method to, as accurately as possible, 'fill in the gaps' between BP cuff measurements. This is critically important, as patient BP can vary significantly at the time-scale of 30 minute measurement samples.

For processes such as this, which are fundamentally repetitive or cyclical by nature and resemble a *batch process* delineated by cuff measurements, iterative learning approaches are generally tractable approaches to modeling and control [21]. These approaches are generally applied to the problem of repetitive *reference tracking* control for example in the manufacturing of semiconductors [22]. In the application described here, the methodology (Fig. 4) will be adapted to form a model-based BP estimator. Estimation of BP is based on measured arterial line pressure, however, an accurate measurement of BP to update the model parameters is only infrequently available (at best every 30 mins). *Run-to-run* control was developed during the 1990s [23], [24] for this class of repetitive batch process. The model structure can take any form, however linear regressions and response surface structures are generally implemented [25], which assume that the process drift is slow enough to compensate with parameter updates when measurements become available. In this application, a model parameter update becomes available at the instant of BP cuff measurement.

A linear regression model of the form

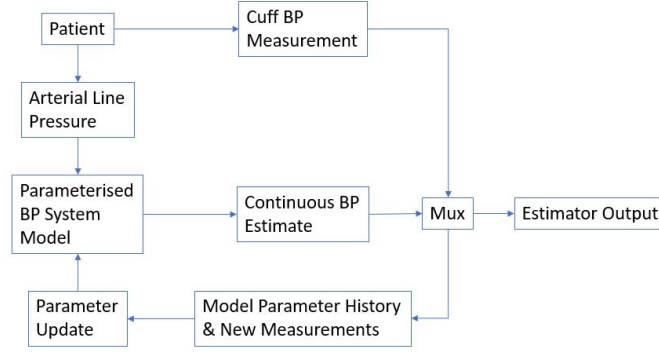


Fig. 4. BP estimator system

$$y(t) = ax(t) + b(t) + \epsilon(t) \quad (2)$$

is generally implemented, where $t = 1, 2, \dots$ denotes the time index; y is the model output, estimated BP in $mmHg$; x is the input, measured arterial line pressure in $mmHg$; a is the *slope coefficient*; b is the *drift coefficient*, and ϵ is the disturbance coefficient. The update objective for y is y^* , and if a and b are accurately known, then the optimal model for the system is

$$x(t) = a^{-1}(y^* - b(t)) \quad (3)$$

Model inaccuracies when compared to the system are inevitable, particularly given the non-stationary nature of the physiological process, unmodelled nonlinearities and stochastic events. Consequently, an iterative parameter adjustment is implemented to update the estimation of a and b

$$b(t) = \lambda[y(t-1) - ax(t-1)] + ((1-\lambda)b(t-1)) \quad (4)$$

which is an exponentially weighted moving average filter [22], tuned by adjusting variable λ in the interval $0 < \lambda < 1$. Combining (4) with (3) gives

$$\begin{aligned} b(t) &= \lambda[y(t-1) - AA^{-1}[y^* - b(t-1)]] + (1-\lambda)b(t-1) \\ b(t) &= b(t-1) + \lambda[y(t-1) - y^*] \end{aligned} \quad (5)$$

which, in its general form is

$$x(t) = \alpha x(t-1) - r(t) \quad (6)$$

where $0 < \alpha < 1$ and $r(t)$ are respectively the *forgetting factor* and *update law* for the model. Typically the system gain a is modeled in advance via designed experiment [26]. In the case under consideration here, the fitted linear relationship for the study population has been derived (eq.1) as $y = 0.8x - 1.5e + 02$ where x is the measured variable *Brachial cuff BP* and y is the corresponding output variable *Arterial Line Pressure*. Given its successful history in the design and implementation of controllers for batch processes, the methodology has been applied to the design of a real-time BP estimator, which is described in the next section.

III. METHOD

In total 12 participants were recruited with 11 completed monitored dialysis sessions. 1 participant moved out of area before a session could be completed. 58.3% of participants were male, with a median age of 65 (IQR 48-78). All participants had continuous non-invasive monitoring of haemodynamics using pulse wave analysis (Finapres NOVA) during a single dialysis treatment of typically 4 hours duration, and data periodically verified by intermittent arm-cuff measurements. Two pressure sensors were attached to the dialysis lines: one between the arterial dialysis needle and dialysis line and the other directly onto the venous-line bubble trap. Data was continuously recorded from all sensors at a sampling rate of 1kHz.

The study protocol was approved by the West Midlands - Coventry and Warwickshire Research Ethics Committee and participants gave written informed consent.

A typical real-time data set for a patient study is shown in Figure 5. Measurements taken during the observational study are acquired and stored for each patient as data sets containing the following datastreams sampled at $1kHz$ and covering the entire treatment period, typically 4 hours;

- Time: continuous from National Instruments board
- Arterial line pressure: continuous from pressure sensor
- Venous line pressure: continuous from pressure sensor
- Occluding cuff BP: intermittent from Finapres Nova
- Reconstructed systolic, diastolic and mean arterial pressure: continuous from Finapres Nova finger cuff

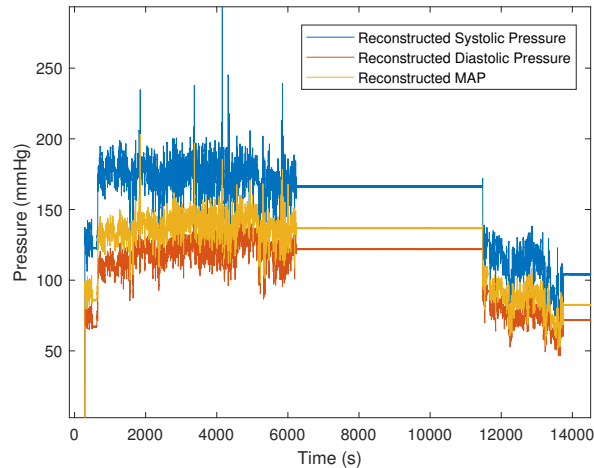


Fig. 5. Typical patient real-time data - reconstructed systolic, diastolic and mean arterial pressure (IT54)

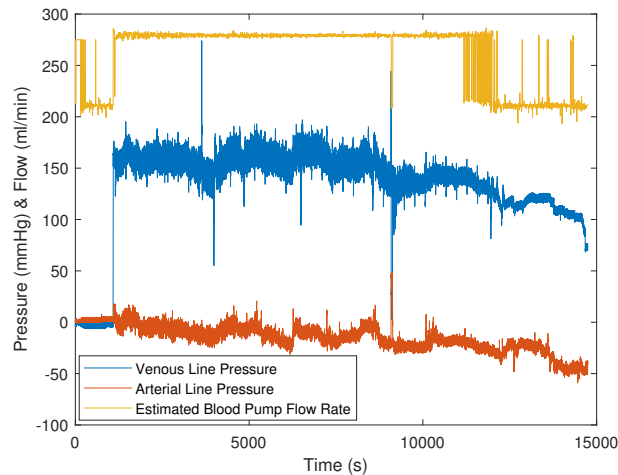


Fig. 6. Typical patient real-time data - venous and arterial line pressure, estimated blood pump flow rate (IT54)

We will now consider the data from a single typical treatment session for patient IT54. Figure (5) shows the reconstructed systolic, diastolic and mean arterial pressures calculated by the Finapres Nova unit from a vascular unloading finger cuff. It is found in practice that this method causes patient discomfort which generally precludes continuous use, hence in this case approximately 2 hours of data at the beginning of treatment and 30 mins of data at the end of treatment are recorded. This was the case for all of the participants in the study, with 30 minute sessions being the average period for finger cuff measurements before the device causes discomfort. Additionally, as the cuff is fitted to a finger on the non-dialysing arm, it can also interfere with run-of-the-mill activities such as refreshment breaks and reading.

Figure (6) shows the directly measured venous and arterial line pressures, along with estimated blood pump flow rate which is derived from the venous line pressure data.

Figure (6) reveals a venous line pressure waveform which is time varying with respect to both mean and amplitude. This measurement is taken at a port on the venous bubble trap which is situated close to the dialyser blood pump. As is to be expected, the waveform dynamics are dominated by the action of the two lobes of this peristaltic pump Fig. (7). This dominating waveform shape should be closely related to the angular speed of the pump and hence should support the derivation of flow rate through the dialysis lines. The time varying nature of the waveform renders this derivation potentially problematic, leading to

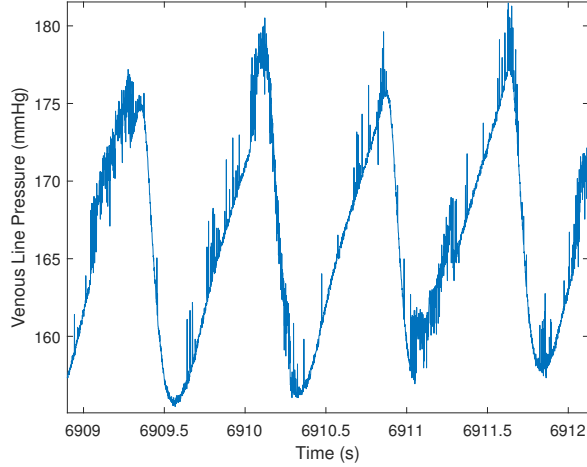


Fig. 7. Typical patient real-time data - venous line pressure detail (IT54)

the application of Fourier modelling to calculate the fundamental frequency of the pump. This method supports the derivation of instantaneous, and hence, time varying pump speed [27]. The problem can be posed as a moving window length L over the real-time venous line pressure data stream which is periodic over the interval $0 \geq x \leq L$, then $f(x)$ can be derived as

$$f(x) = a_0 + \sum_{n=1}^{\infty} \left[a_n \cos\left(\frac{2\pi nx}{L}\right) + b_n \sin\left(\frac{2\pi nx}{L}\right) \right] \quad (7)$$

which is the *Fourier trigonometric series for the function* $f(x)$. In the case under examination here, the fundamental frequency of the blood pump is sought, so calculations are constrained to $n = 1$.

Examination of Figs. (5 - 7) reveals waveforms which comprise cyclical elements which are varying in both amplitude and mean in addition to measurement noise. In order to smooth the signals to facilitate real time calculations, moving average filters with a window length of *5000 samples* or *5s* was implemented on all data lines with the exception of BP which has a single value at each measurement event. The window length was chosen as being over twice the length of the period of a slow heart rate (HR) of 30bpm in order to avoid aliasing. The pump frequency is calculated and updated in real-time over this sliding window. Additionally, arm cuff measurements are characterised as steady-state phenomena as they are discrete measurements without dynamics. Derived pump frequency is converted to flow in units of mls^{-1} by

$$fl = \left(\left(\frac{fr(rads^{-1})}{2\pi} \right) \times 60 \right) \times (\pi r^2 Ln) \quad (8)$$

where fl is flow in mls^{-1} , fr is pump frequency in $rads^{-1}$, r is the radius of the dialysis line within the pump in mm and Ln is the effective length of line within the pump in mm . In the example shown in Fig. (6) the estimate of $290ml/min$ agrees with the flow rate recorded in the patient's record.

Filtered mean arterial line pressure and reconstructed arterial waveforms are shown in Fig. (8) with corresponding arm cuff MAP measurements during the treatment period.

Real-time code has been developed in Matlab/Simulink [28] to perform calculations on patient measurement data streams acquired during dialysis treatment. The algorithm is structured as follows;

- 1) pre-calculate recursive least fit for the patient populations previously measured and recorded BP - arterial line pressure pairs Fig. (2). In this case, with x as the measured variable *arterial line pressure* and y as the predictor variable *BP*, we derive the relationship of the form $y(t) = ax(t) + b(t) + \epsilon(t)$ Eq. 2 as $y = 0.619x + 138.8 + \epsilon$
- 2) the a coefficient in Eq.(2) is thus fixed as 0.619 for this patient and will be updated for future treatments as more data is acquired
- 3) initial estimates of BP are conducted with the population derived fit until the first new BP/line pressure measurement is received
- 4) the relationship $y(t) = ax(t) + b(t) + \epsilon(t)$ is updated according to Eq. 4
- 5) estimates of BP are conducted with the updated estimator
- 6) new measurements received
- 7) repeat from item 4

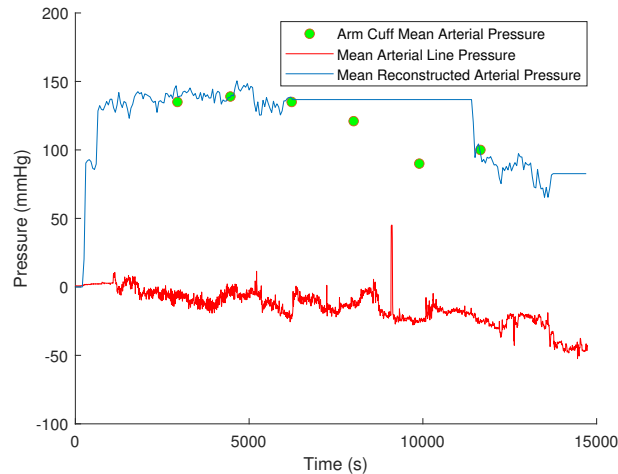


Fig. 8. Typical patient real-time data - occluding arm cuff pressure, mean arterial line pressure, mean reconstructed arterial pressure (IT54)

TABLE I
BASELINE PARTICIPANT CHARACTERISTICS

VARIABLE	(n=7)
Age (years)	53 (*IQR 49 to 70)
Male [n (%)]	3 (43)
White ethnicity [n (%)]	5 (71)
Current smoking [n (%)]	1 (14)
Diabetes [n (%)]	2 (29)
Ischaemic heart disease [n (%)]	2 (29)
Dialysis vintage (months)	6 (6 to 23)
Dialysis adequacy (Kt/V)	1.24 (0.97 to 1.46)
Fistula blood flow assessment (QA)	670 (635 to 1072)
<i>Vascular access type</i>	
Brachiocephalic arteriovenous fistula [n (%)]	4 (57)
Radiocephalic arteriovenous fistula [n (%)]	3 (43)
<i>Needle gauge</i>	
2x 14g [n (%)]	3 (43)
2x 15g [n (%)]	3 (43)
Arterial 15g; Venous 16g [n (%)]	1 (14)
Post-dialysis weight (kg)	78.6 (64.1 to 98.2)
Body mass index (kg/m^2)	26.3 (24.4 to 34.4)
*IQR, interquartile range	

IV. RESULTS

9 complete treatment data sets were processed and subsequently analysed, characteristics of the patients in the study are given in Table I

Fig. 9 shows the typical updating of the model over an approximately 4-hour treatment period as new BP/line pressure measurements are acquired.

The associated BP estimator for this treatment is shown in Fig. 10. Blood pump flow for this treatment is consistent at $280ml/min$.

The initial estimate at 3500s is based upon the initial population fit model and exhibits a relatively wide divergence from the incoming accurate BP measurement. Subsequent pairs show the incoming BP measurement, with the estimate from the predictor model prior to update, and exhibit improved accuracy when compared to the first estimate in all patients.

Performance of the estimator scheme for patients in the study is shown in Table II. Maximum errors are exclusively associated with the initial estimates derived from the population model. Errors then tend to decrease significantly after the first BP update. The average RMS error for all the sessions analysed here (including initial modelling error) is $11.5mmHg$. Eliminating the initial modeling error reduces the average RMS error to $7.9mmHg$

Finally for completeness, we can examine the performance of the estimator against dynamic, continuous BP measurement (Fig. 11). There is reasonable performance in tracking the cuff BP measurements, however, with the continuous BP measurement provided by the Fiapres Nova finger cuff there are obvious shortcomings. This is to be expected when comparing the performance of a steady-state linear model against the output of a dynamic non-linear system.

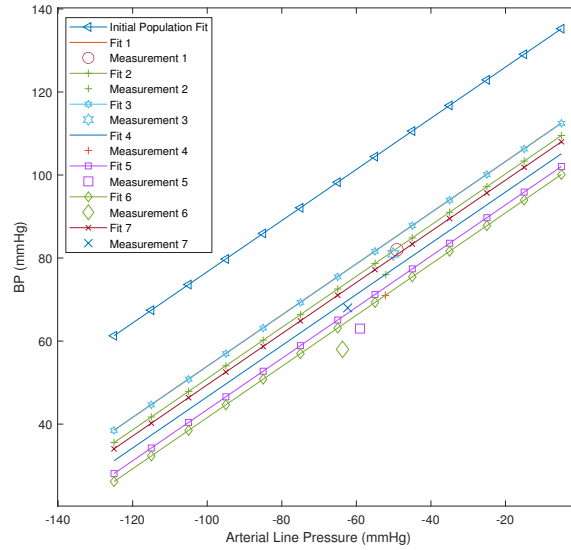


Fig. 9. IT62 Initial population fit predictor, incoming measurements and predictor updates over 4 hour treatment

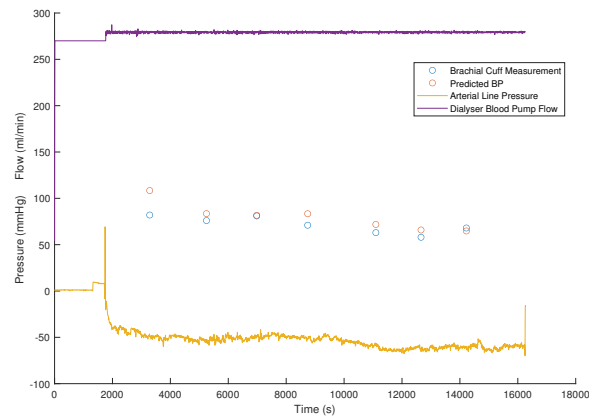


Fig. 10. IT62 measured and predicted BP, arterial line pressure and blood pump flow over 4 hour treatment

V. CONCLUSION

A non-invasive, recursive BP estimator has been designed and analysed on real-time data sets from an observational patient study. The parameterised run-to-run adaptive model described is initially fitted to data from the study population, and subsequently updated with the individual's line and BP data when it is available. The problem of defining initial conditions for the estimator model and reliance on sparse update data is extremely challenging. There are a number of significant outcomes

TABLE II
ESTIMATOR PERFORMANCE OVER TREATMENT SESSIONS WHEN COMPARED TO INCOMING BP MEASUREMENTS (MMHG)

Patient	RMS Error	Max Error	Min Error
IT62	12.27	26.38	0.71
IT58	7.47	14.89	2.08
IT57	11.19	21.17	0.38
IT54	28.48	51.45	1.7
IT62	11.51	28.68	0.38
IT60	7.47	18.9	1.22
IT57	12.94	25.68	1.06
IT56	6.76	13.08	0.77
IT55	5.56	14.33	2.01

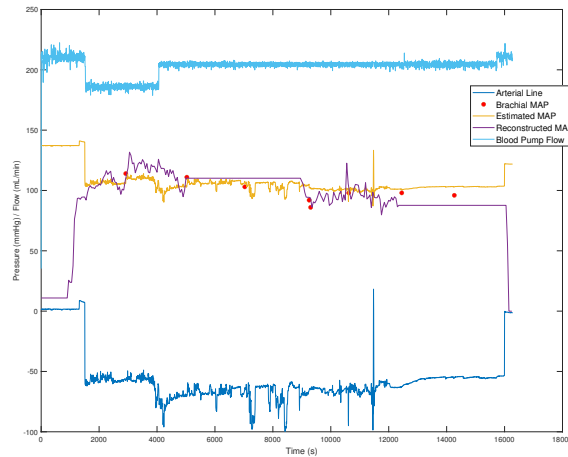


Fig. 11. IT57 measured and predicted static and dynamic BP, arterial line pressure and blood pump flow over 4 hour treatment

from this phase of the research programme. Firstly, in this study, and a previous 50 patient study which examined heart rate and blood pressure variability in dialysis treatment [29], it is apparent that continuous monitoring technology currently faces challenges in applications with long treatment times. The method described in this paper successfully conducts estimation of BP based only on the pressure measurements from sensors placed in the dialysis lines, and intermittent BP measurements. As such it fulfills the requirements of a usable non-invasive, continuous estimator.

In its current form, the estimator can track trends in patient BP albeit with an average RMS error of 7.9mmHg between prediction and updated BP measurement. Consequently, it represents a significant step forward in this area as the ability to repeatably track changes in BP rather than measure instantaneous BP with high levels of accuracy is currently a critical necessity during treatment. Examination of Fig. 11 reveals the mismatch between the performance of the linear steady-state model and the non-linear dialyser-physiological patient dynamics. Future work will develop a non-linear parameterised model estimator, which will still utilise measured BP updates, but will have more reliance on the complex interaction between the venous and arterial lines real-time pressure measurements. In this way, the model will have less reliance on a population model for initial conditions, and in particular will be able to estimate both steady-state and dynamic BP response, which should enable more accurate real-time estimates rather than trend estimation from the current estimation scheme.

ACKNOWLEDGMENTS

The authors would like to thank Mel Morris and the MStart Foundation for funding the iTrend research programme, and the support of the Royal Derby Hospital Renal Unit.

US Patent Office & Overseas License 62/855069 MEASURING PRESSURE WAVES IN DIALYSIS LINES TO DERIVE CONTINUOUS ARTERIAL BLOOD PRESSURE Prof Paul Stewart, Prof Jill Stewart, et al. iTrend Medical Research Ltd.

REFERENCES

- [1] A. Meidert and B. Saugel, *Techniques for Non-Invasive Monitoring of Arterial Blood Pressure*, Front Med (Lausanne). 2017; 4: 231. Published online 2018 Jan 8. doi: 10.3389/fmed.2017.00231.
- [2] J. Bijker, S. Persoon, L. Peelen, K. Moons, C. Kalkman, L. Kappelle, et al. *Intraoperative hypotension and perioperative ischemic stroke after general surgery: a nested case-control study*, Anesthesiology (2012) 116:658–64.10.1097/ALN.0b013e3182472320
- [3] J. van Waes, W. van Klei, D. Wijeyundera, L. van Wolfswinkel, T. Lindsay, W. Beattie, *Association between intraoperative hypotension and myocardial injury after vascular surgery*, Anesthesiology (2016) 124:35–44.10.1097/ALN.0000000000000922
- [4] M. Walsh, P. Devereaux, A. Garg, A. Kurz, A. Turan, R. Rodseth, et al., *Relationship between intraoperative mean arterial pressure and clinical outcomes after noncardiac surgery: toward an empirical definition of hypotension*, Anesthesiology (2013) 119:507–15.10.1097/ALN.0b013e3182a10e26
- [5] Flythe et al Association of mortality risk with various definitions of intradialytic hypotension, J Am Soc Nephrol. 2015 Mar;26(3):724-34. doi: 10.1681/ASN.2014020222. Epub 2014 Sep 30.
- [6] G. Mahe, E. Comets, A. Nouni, F. Paillard, C. Dourmap, A. Le Faucheur and V. Jaquinandi, *A minimal resting time of twenty five minutes is needed before measuring stabilized blood pressure in subjects addressed for vascular investigations*, Scientific Reports volume 7, Article number: 12893 (2017)
- [7] G. Pressman and P. Newgard, *A transducer for the continuous external measurement of arterial blood pressure*, IEEE Trans Biomed Eng (1963) 10:73–81.
- [8] A. Meidert, W. Huber, A. Hapfelmeier, M. Schöfthaler, J. Müller, N. Langwieser, et al., *Evaluation of the radial artery applanation tonometry technology for continuous noninvasive blood pressure monitoring compared with central aortic blood pressure measurements in patients with multiple organ dysfunction syndrome*, J Crit Care (2013) 28:908–12.10.1016/j.jcrc.2013.06.012
- [9] B. Saugel, R. Dueck and J. Wagner. *Measurement of blood pressure*, Best Pract Res Clin Anaesthesiol (2014) 28:309–22.10.1016/j.bpa.2014.08.001

- [10] R. Dueck, O. Goedje and P. Clopton. *Noninvasive continuous beat-to-beat radial artery pressure via TL-200 applanation tonometry*, J Clin Monit Comput (2012) 26:75–83. [10.1007/s10877-012-9336-2](https://doi.org/10.1007/s10877-012-9336-2)
- [11] J. Penaz, A. Voigt and W. Teichmann. *Contribution to the continuous indirect blood pressure measurement*, Z Gesamte Inn Med (1976) 31:1030–3
- [12] Wang R, Jia W, Mao ZH, Scلابassi RJ, Sun M. Cuff-Free Blood Pressure Estimation Using Pulse Transit Time and Heart Rate, Int Conf Signal Process Proc. 2014;2014:115–118. [doi:10.1109/ICOSP.2014.7014980](https://doi.org/10.1109/ICOSP.2014.7014980)
- [13] Meidert Agnes S., Saugel Bern Techniques for Non-Invasive Monitoring of Arterial Blood Pressure Frontiers in Medicine, 5, 231, 2018
- [14] C. Rhee, Y. Obi, A. Mathew and K. Kalantar-Zadeh, *Precision Medicine in the Transition to Dialysis and Personalized Renal Replacement Therapy*, Semin Nephrol. 2018 Jul;38(4):325-335. [doi: 10.1016/j.semnephrol.2018.05.003](https://doi.org/10.1016/j.semnephrol.2018.05.003).
- [15] G. Piccoli, L. Nielsen, L. Gendrot, A. Fois, E. Cataldo and G. Cabiddu, *Prescribing Hemodialysis or Hemodiafiltration: When One Size Does Not Fit All the Proposal of a Personalized Approach Based on Comorbidity and Nutritional Status*, settings J. Clin. Med. 2018, 7(10), 331; <https://doi.org/10.3390/jcm7100331>
- [16] R. Agarwal, T. Metiku, G. G. Tegegne, R. P. Light, Z. Bunaye, D. Bekele and K. Kelley, *Diagnosing Hypertension by Intradialytic Blood Pressure Recordings*, Clin J Am Soc Nephrol. 2008 Sep; 3(5): 1364–1372. [doi: 10.2215/CJN.01510308](https://doi.org/10.2215/CJN.01510308)
- [17] M. Assimon, and J. Flythe, *Intradialytic blood pressure abnormalities: the highs, the lows, and all that lies between*, Am J Nephrol. 2015; 42(5): 337–350. Published online 2015 Nov 20. [doi: 10.1159/000441982](https://doi.org/10.1159/000441982)
- [18] Stewart, Jill, Paul Stewart, Thomas Walker, Tarek Eldehni, Daniela V. Horner, Bethany Lucas, Kelly White, et al. 2020. *A Feasibility Study of Non-invasive Continuous Estimation of Brachial Pressure Derived from Arterial and Venous Lines During Dialysis* engrXiv. May 7. [doi:10.31224/osf.io/xpv65](https://doi.org/10.31224/osf.io/xpv65)
- [19] P. Stewart, J. Stewart, T. Walker, L. Gullapudi, N. Selby and M. Taal, *Measuring pressure waves in dialysis lines to derive continuous arterial blood pressure: pilot work in an in vitro and in silico model* Nephrology Dialysis Transplantation, Volume 34, Issue Supplement 1, June 2019, [gfz103.SP541](https://doi.org/10.1093/ndt/gfz103.SP541), <https://doi.org/10.1093/ndt/gfz103.SP541> Published: 13 June 2019
- [20] P. Stewart, J. Stewart, T. Walker, L. Gullapudi, M. Taal and N. Selby, *Development of an in vitro simulation model to investigate haemodynamic responses during haemodialysis*, Nephrology Dialysis Transplantation, Volume 34, Issue Supplement 1, June 2019, [gfz106.FP630](https://doi.org/10.1093/ndt/gfz106.FP630), <https://doi.org/10.1093/ndt/gfz106.FP630> Published: 13 June 2019
- [21] Youqing Wang, Furong Gao and Francis J. Doyle III, *Survey on iterative learning control, repetitive control, and run-to-run control*, Journal of Process Control, Volume 19, Issue 10, December 2009, Pages 1589-1600, <https://doi.org/10.1016/j.jprocont.2009.09.006>
- [22] Moyne J. (2014) *Run-to-Run Control in Semiconductor Manufacturing*. In: Baillieul J., Samad T. (eds) Encyclopedia of Systems and Control. Springer, London
- [23] E. Sachs, R.-S. Guo, S. Ha and A. Hu, *On-line process optimization and control using the sequential design of experiments*, Digest of Technical Papers.1990 Symposium on VLSI Technology, Honolulu, Hawaii, USA, 1990, pp. 99-100, [doi: 10.1109/VLSIT.1990.111027](https://doi.org/10.1109/VLSIT.1990.111027).
- [24] E. Sachs, R.-S. Guo, S. Ha and A. Hu, *Process control system for VLSI fabrication*, in *IEEE Transactions on Semiconductor Manufacturing*, vol. 4, no. 2, pp. 134-144, May 1991, [doi: 10.1109/66.79725](https://doi.org/10.1109/66.79725).
- [25] William Jarrett Campbell, Stacy Firth, Anthony Toprac, Thomas F. Edgar, *A comparison of Run-to-Run Control algorithms*, Proceedings of the American Control Conference 3:2150 - 2155 vol.3 DOI: 10.1109/ACC.2002.1023955
- [26] G.P.Box, W.G. Hunter and J.S. Hunter, *Statistics for Experimenters: An Introduction to Design, Data Analysis, and Model Building*, John Wiley and Sons Inc., New York, 1st ed., 1978.
- [27] I. López-García, M. Sánchez-Merlos, P. Viñas, M. Hernández-Córdoba, *Peristaltic pumps-Fourier transforms: a coupling of interest in continuous flow flame atomic absorption spectrometry*, Spectrochimica Acta Part B: Atomic Spectroscopy, Volume 51, Issue 14, 1996, Pages 1761-1768, ISSN 0584-8547, [https://doi.org/10.1016/S0584-8547\(96\)01557-1](https://doi.org/10.1016/S0584-8547(96)01557-1). (<http://www.sciencedirect.com/science/article/pii/S0584854796015571>)
- [28] <https://uk.mathworks.com/products/matlab.html>
- [29] J. Stewart, P. Stewart, T. Walker, L. Gullapudi, T. Eldehni, N. Selby et al. (2020), *An Application of The Lomb-Scargle Periodogram To Investigate Heart Rate Variability During Haemodialysis* TechRxiv. Preprint. <https://doi.org/10.36227/techrxiv.12442181.v1>